



Proudly Owned and Operated in the USA

Searchable via: [FreedomDiagnosticsTesting.com](https://freedomdiagnostics.com)

Product	GLP-3 RT 5mg
Net Peptide Content	Vial 1: 5.22 mg Vial 2: 5.45 mg
Average Net Peptide	5.34 mg

Certificate of Analysis

Accession Number	2512020022
Client	Nova Peptides
Search Code	Nova2512020022



Received Date:	12/02/2025
Reported Date:	12/4/2025

Lot	NV-P-5AAZ
Purity	Vial 1: 99.617% Vial 2: 99.715%
Appearance	White Lyophilized Powder

Endotoxin Threshold		Result
Replicate 1	≤ 0.05 EU/mL	PASS
Replicate 2	≤ 0.05 EU/mL	PASS

All Chemical Analysis was performed by HPLC with UV Detection Coupled with Mass Spectrometry

Mass Identification	Result
GLP-RT	99.67%

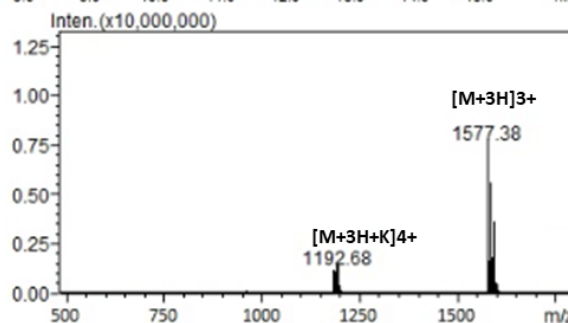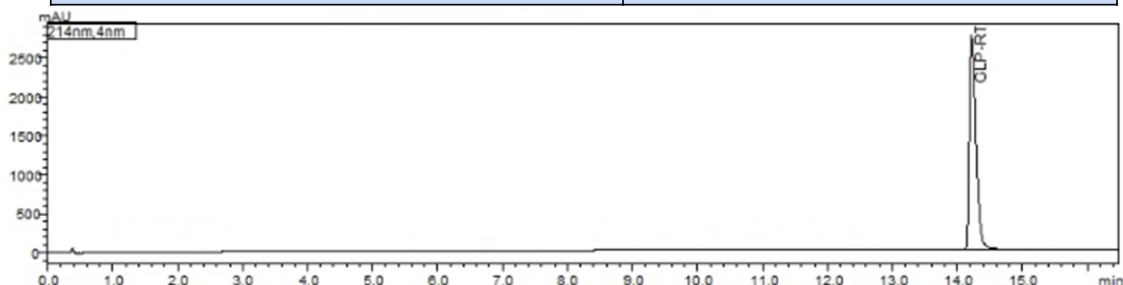

Stephen Schmidt

Stephen Schmidt
Principal Chemist

COA: 2512020022

The peptide purity analysis reported here was conducted using LCMS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.

Searchable via: [FreedomDiagnosticsTesting.com](https://freedomdiagnostics.com)

Contact at: Admin@FreedomDiagnostics.net



Proudly Owned and Operated in the USA

Searchable via: [FreedomDiagnosticsTesting.com](https://freedomdiagnostics.com)

Product	GLP-3 RT 5mg
Net Peptide Content	Vial 1: 5.76 mg Vial 2: 5.69 mg
Average Net Content	5.725 mg

Certificate of Analysis

Accession Number	2601210055
Client	Nova Peptides
Search Code	Nova2601210055



Received Date:	01/21/2026
Reported Date:	1/22/2026

Lot	NV-P-5AAZ
Purity	Vial 1: 99.42% Vial 2: 99.521%
Appearance	White Lyophilized Powder

Endotoxin Threshold		Result
Replicate 1	≤ 0.5 EU/mg	PASS
Replicate 2	≤ 0.5 EU/mg	PASS

All Chemical Analysis was performed by HPLC with UV Detection Coupled with Mass Spectrometry

Mass Identification	Result
GLP RT	99.47%

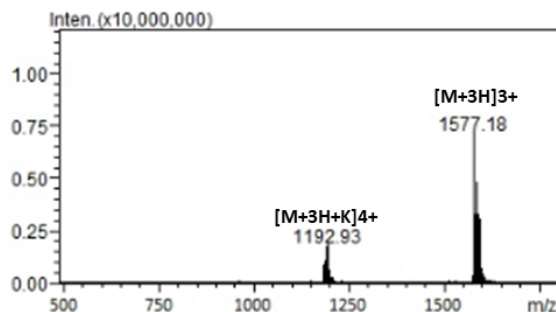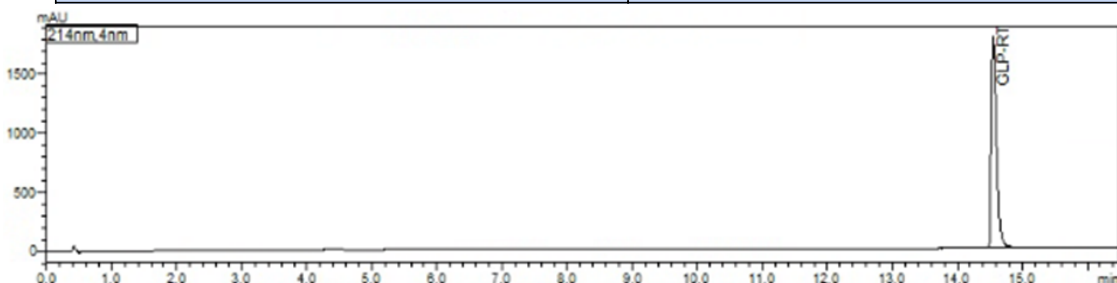

Stephen Schmidt

Stephen Schmidt
Principal Chemist

COA: 2601210055

The peptide purity analysis reported here was conducted using LCMS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.

Searchable via: [FreedomDiagnosticsTesting.com](https://freedomdiagnostics.com)

Contact at: Admin@FreedomDiagnostics.net